

# Model 401B04 SPECS 401B04 SERIES Installation and Operating Manual

For assistance with the operation of this product, contact PCB Piezotronics, Inc.

Toll-free: 800-828-8840 24-hour SensorLine: 716-684-0001

> Fax: 716-684-0987 E-mail: info@pcb.com Web: www.pcb.com







# Warranty, Service, Repair, and Return Policies and Instructions

The information contained in this document supersedes all similar information that may be found elsewhere in this manual.

**Total Customer Satisfaction** – PCB Piezotronics guarantees Total Customer Satisfaction. If, at any time, for any reason, you are not completely satisfied with any PCB product, PCB will repair, replace, or exchange it at no charge. You may also choose to have your purchase price refunded in lieu of the repair, replacement, or exchange of the product.

**Service** – Due to the sophisticated nature of the sensors and associated instrumentation provided by PCB Piezotronics, user servicing or repair is not recommended and, if attempted, may void the factory warranty. Routine maintenance, such as the cleaning of electrical connectors, housings, mounting surfaces with solutions and techniques that will not harm the physical material of construction, is acceptable. Caution should be observed to insure that liquids are not permitted to migrate into devices that are not hermetically sealed. Such devices should only be wiped with a dampened cloth and never submerged or have liquids poured upon them.

**Repair** – In the event that equipment becomes damaged or ceases to operate, arrangements should be made to return the equipment to PCB Piezotronics for repair. User servicing or repair is not recommended and, if attempted, may void the factory warranty.

**Calibration** – Routine calibration of sensors and associated instrumentation is

recommended as this helps build confidence in measurement accuracy and acquired data. Equipment calibration cycles are typically established by the users own quality regimen. When in doubt about a calibration cycle, a good "rule of thumb" is to recalibrate on an annual basis. It is also good practice to recalibrate after exposure to any severe temperature extreme, shock, load, or other environmental influence, or prior to any critical test.

PCB Piezotronics maintains an ISO-9001 certified metrology laboratory and offers calibration services, which are accredited by A2LA to ISO/IEC 17025, with full traceablility to N.I.S.T. In addition to the normally supplied calibration, special testing is also available, such as: sensitivity at elevated cryogenic temperatures, phase extended response, high frequency response, extended range, leak testing, hydrostatic pressure testing, and others. For information on standard recalibration services or special testing, contact your local PCB Piezotronics distributor, sales representative, factory customer service representative.

Returning Equipment – Following these procedures will insure that your returned materials are handled in the most expedient manner. Before returning any equipment to PCB Piezotronics, contact your local distributor, sales representative, or factory customer service representative to obtain a Return

Materials Authorization (RMA) Number. This RMA number should be clearly marked on the outside of all package(s) and on the packing list(s) accompanying the shipment. A detailed account of the nature of the problem(s) being experienced with the equipment should also be included inside the package(s) containing any returned materials.

A Purchase Order, included with the returned materials, will expedite the turn-around of serviced equipment. It is recommended to include authorization on the Purchase Order for PCB to proceed with any repairs, as long as they do not exceed 50% of the replacement cost of the returned item(s). PCB will provide a price quotation or replacement recommendation for any item whose repair costs would exceed 50% of replacement cost, or any item that is not economically feasible to repair. For routine calibration services, the Purchase Order should include authorization to proceed and return at current pricing, which can be obtained from a factory customer service representative.

Warranty – All equipment and repair services provided by PCB Piezotronics, Inc. are covered by a limited warranty against defective material and workmanship for a period of one year from date of original purchase. Contact PCB for a complete statement of our warranty. Expendable items, such as batteries and mounting hardware, are not covered by warranty. Mechanical damage to equipment due to improper use is not covered by warranty. Electronic circuitry failure caused by the introduction of unregulated or improper excitation power or electrostatic discharge is not covered by warranty.

**Contact Information** – International customers should direct all inquiries to their local distributor or sales office. A complete list of distributors and offices be found at www.pcb.com. Customers within the United States may contact their local sales representative or customer factory service representative. A complete list of sales representatives can be found www.pcb.com. Toll-free telephone numbers for a factory customer service representative, in the division responsible for this product, can be found on the title page at the front of this manual. Our ship to address and general contact numbers are:

PCB Piezotronics, Inc. 3425 Walden Ave. Depew, NY 14043 USA Toll-free: (800) 828-8840

24-hour SensorLine<sup>SM</sup>: (716) 684-0001

Website: www.pcb.com E-mail: info@pcb.com

DOCUMENT NUMBER: 21354 DOCUMENT REVISION: B

ECN: 17900



# 401B04 ICP® Sensor Simulator

# 1. INTRODUCTION AND DESCRIPTION

The Model 401B04 is a unity gain, non-inverting, impedance-converting voltage amplifier with the same characteristics as the built-in ICP® amplifiers provided in most PCB pressure sensors, force sensors, and accelerometers. This model consists of MOSFET circuitry packaged in a convenient Pomona box with BNC connectors. When used in conjunction with a signal generator or oscillator, it can be used in place of an ICP sensor to calibrate ICP® sensor signal conditioners, do system verifications and gain adjustments, or check frequency response of systems with long input cables. (The Model 401B04 simulates the circuit of an ICP® sensor while the signal generator takes the place of the sensor's crystals.)

# 2. INSTALLATION AND OPERATION


CAUTION: Connect the output only to an ICP® type, current-limited signal conditioner.

WARNING: Excessive current may damage this model. Measure the ICP<sup>®</sup> sensor signal conditioner current prior to connecting the 401B04. The ICP<sup>®</sup> excitation current should be ≤20 mA.

# 2.1 CALIBRATION OF ICP® SENSOR SIGNAL CONDITIONERS

Refer to the acceptance test procedure for your particular PCB signal conditioner, dual mode charge amplifier, or digital peak meter model. (Acceptance test procedures are available for most PCB electronic products. Consult factory for details.)

Connect a signal generator or oscillator to the input jack of the 401B04, after observing the caution and warning above. Connect the output jack of the 401B04 to the ICP® sensor signal conditioner being tested. (Various cables and adaptors are available from PCB as needed.) Switch on the signal conditioner and note the output bias voltage on the meter as you would for any ICP® sensor. The meter should read mid scale, indicating that the 401B04 is operational. Follow the acceptance test procedure for your particular PCB model. The exact gain factor (near unity) of the 401B04 is noted on the calibration certificate supplied with the unit. The nominal value of Gain = 1.0 is on the housing of the unit.

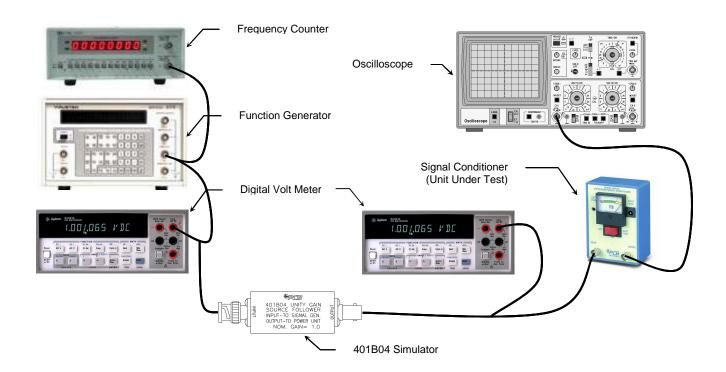



# 2.2 MEASUREMENT SYSTEM CHECKOUT AND/OR GAIN ADJUST

The Model 401B04 is inserted in place of the ICP<sup>®</sup> sensor in your measurement system. Connect the input of the 401B04 to a signal generator and the output to the ICP<sup>®</sup> sensor signal conditioner. Also connect any additional amplifiers or recording devices that will be used in the test, as shown in the figure above. After switching on all equipment and allowing sufficient warm-up time, apply a known signal through the system with the signal generator and adjust gains, ranges, zeroes, etc., as needed.

# 2.3 CALIBRATION OF LONG LINES

Model 401B04 can be used, in conjunction with an oscillator or step function generator, to simulate an ICP® sensor driving a long input cable between the sensor and the ICP sensor signal conditioner. Refer to PCB "General Guide to ICP® Instrumentation" for more details on the procedure.

# 3. FREQUENCY RESPONSE CONSIDERATIONS

When used with a signal generator for system checkouts or testing of long lines, low frequency response of the 401B04 is DC.

High frequency response of the Model 401B04, when driving short cables with small (~1V) signals, is 1 megahertz. Refer to PCB "General Guide to ICP® Instrumentation." if long cables are to be driven. Also, consult the factory if less than 2 mA constant current will be used to power the 401B04.

# 4. MEASUREMENT AND REPAIR

The miniature size precludes most maintenance. If used in a very humid or dirty environment, signal degradation, usually in the form of reduced output or loss of low frequency response, may occur. If the connectors become dirty, clean with Freon TF ®, Genesolv, or other suitable solvent that leaves no residue.

Manual Number: 40858 Manual Revision: A ECN Number: 38393



# 401B04 ICP® Sensor Simulator

# 1. INTRODUCTION AND DESCRIPTION

The Model 401B04 is a unity gain, non-inverting, impedance-converting voltage amplifier with the same characteristics as the built-in ICP® amplifiers provided in most PCB pressure sensors, force sensors, and accelerometers. This model consists of MOSFET circuitry packaged in a convenient Pomona box with BNC connectors. When used in conjunction with a signal generator or oscillator, it can be used in place of an ICP sensor to calibrate ICP® sensor signal conditioners, do system verifications and gain adjustments, or check frequency response of systems with long input cables. (The Model 401B04 simulates the circuit of an ICP® sensor while the signal generator takes the place of the sensor's crystals.)

# 2. INSTALLATION AND OPERATION


CAUTION: Connect the output only to an ICP® type, current-limited signal conditioner.

WARNING: Excessive current may damage this model. Measure the ICP<sup>®</sup> sensor signal conditioner current prior to connecting the 401B04. The ICP<sup>®</sup> excitation current should be ≤20 mA.

# 2.1 CALIBRATION OF ICP® SENSOR SIGNAL CONDITIONERS

Refer to the acceptance test procedure for your particular PCB signal conditioner, dual mode charge amplifier, or digital peak meter model. (Acceptance test procedures are available for most PCB electronic products. Consult factory for details.)

Connect a signal generator or oscillator to the input jack of the 401B04, after observing the caution and warning above. Connect the output jack of the 401B04 to the ICP® sensor signal conditioner being tested. (Various cables and adaptors are available from PCB as needed.) Switch on the signal conditioner and note the output bias voltage on the meter as you would for any ICP® sensor. The meter should read mid scale, indicating that the 401B04 is operational. Follow the acceptance test procedure for your particular PCB model. The exact gain factor (near unity) of the 401B04 is noted on the calibration certificate supplied with the unit. The nominal value of Gain = 1.0 is on the housing of the unit.

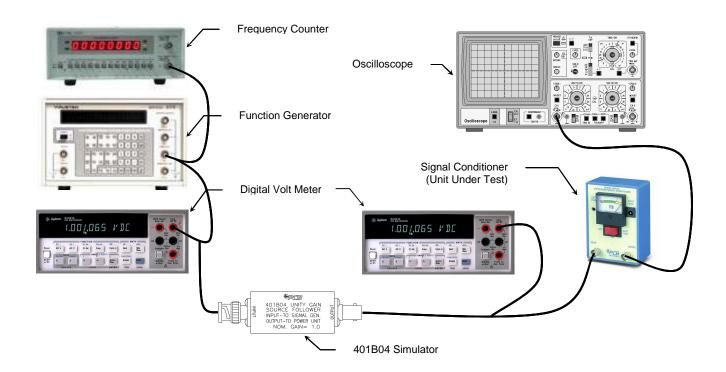



# 2.2 MEASUREMENT SYSTEM CHECKOUT AND/OR GAIN ADJUST

The Model 401B04 is inserted in place of the ICP<sup>®</sup> sensor in your measurement system. Connect the input of the 401B04 to a signal generator and the output to the ICP<sup>®</sup> sensor signal conditioner. Also connect any additional amplifiers or recording devices that will be used in the test, as shown in the figure above. After switching on all equipment and allowing sufficient warm-up time, apply a known signal through the system with the signal generator and adjust gains, ranges, zeroes, etc., as needed.

# 2.3 CALIBRATION OF LONG LINES

Model 401B04 can be used, in conjunction with an oscillator or step function generator, to simulate an ICP® sensor driving a long input cable between the sensor and the ICP sensor signal conditioner. Refer to PCB "General Guide to ICP® Instrumentation" for more details on the procedure.

# 3. FREQUENCY RESPONSE CONSIDERATIONS

When used with a signal generator for system checkouts or testing of long lines, low frequency response of the 401B04 is DC.

High frequency response of the Model 401B04, when driving short cables with small (~1V) signals, is 1 megahertz. Refer to PCB "General Guide to ICP® Instrumentation." if long cables are to be driven. Also, consult the factory if less than 2 mA constant current will be used to power the 401B04.

# 4. MEASUREMENT AND REPAIR

The miniature size precludes most maintenance. If used in a very humid or dirty environment, signal degradation, usually in the form of reduced output or loss of low frequency response, may occur. If the connectors become dirty, clean with Freon TF ®, Genesolv, or other suitable solvent that leaves no residue.

Manual Number: 40858 Manual Revision: A ECN Number: 38393

Model Number <b>401B04</b>			ICP® SOURCE F	OLL	OWER
Performance		ENGLISH	SI		Optional '
Output Range		±5 V	±5 V		for standa
Low Frequency F	Response	0 Hz	0 Hz		
High Frequency I	Response (2.0 mA)	110 kHz	110 kHz	[3]	Notes
High Frequency I	Response (4 mA)	220 kHz	220 kHz	[3]	[1] ا
High Frequency I	Response (20 mA)	1000 kHz	1000 kHz	[3]	[2]
Non-Linearity		≤2 % FS	≤2 % FS		[3] /
Environmental					[4] :
Temperature Rar	nge (Operating)	+30 to +150 °F	0 to +50 °C		con
Electrical					
Excitation Voltage	e	+18 to 30 VDC	+18 to 30 VDC		
Constant Current	Excitation	2 to 20 mA	2 to 20 mA		
Output Current		1 to 19 mA	1 to 19 mA	[1]	
Output Impedance		<100 Ohm	<100 Ohm		
Output Bias Volta	age	+7 to 14 VDC	+7 to 14 VDC		
	rical Noise (1 to 10000	12 μV rms	12 μV rms	[2]	
Hz)					
Spectral Noise (	` '	4 μg/√Hz	4 μg/√Hz	[2]	
Spectral Noise (	(1 Hz)	1 μg/√Hz	1 μg/√Hz	[2]	
Spectral Noise (	(10 Hz)	0.3 μg/√Hz	0.3 μg/√Hz	[2]	
Spectral Noise (	(100 kHz)	0.1 µg/√Hz	0.1 μg/√Hz	[2]	
Spectral Noise (	(1 kHz)	0.05 μg/√Hz	0.05 µg/√Hz	[2]	
Insulation Resista	ance (Minimum )	10 <sup>9</sup> Ohm	10 <sup>9</sup> Ohm		
Physical	,				
Housing Material		Aluminum	Aluminum		
Electrical Connec	ctor (Input)	BNC Plug	BNC Plug		
Electrical Connec	ctor (Output)	BNC Jack	BNC Jack		
Size (Length x W	idth x Height)	2.2 in x 1.1 x 0.9	55.9 mm x 27.9 x 22.9		
Weight	- <i>'</i>	2.50 oz	70.9 gm		

**(€**[4]

All specifications are at room temperature unless otherwise specified.

In the interest of constant product improvement, we reserve the right to change specifications without

ICP® is a registered trademark of PCB group, Inc.

ECN #: 30009 Optional Versions (Optional versions have identical specifications and accessories as listed for standard model except where noted below. More than one option maybe used.)

Revision A

### Notes

- [1] Excitation current supplied minus 1 mA nominal current consumption.
- [2] Typical, tested with 1000 pF capacitance at input.
- [3] Above stated frequency, the amplifier becomes slew rate limited.
- [4] See PCB Declaration of Conformance PS024 for details. A low impendance connection from case to earth ground is required to maintain CE compliance.


Entered: BLS	Engineer: PLH	Sales: JJM	Approved: LLH	Spec Number:
Date:	Date:	Date:	Date:	40857
01/29/2009	01/26/2009	01/26/2009	01/30/2009	





3425 Walden Avenue Depew, NY 14043 UNITED STATES Phone: 800-828-8840 Fax: 716-684-0987 E-mail: info@pcb.com Web site: www.pcb.com PCB Piezotronics Inc. claims proprietary rights in the information disclosed hereon. Neither it nor any reproduction thereof will be disclosed to others without written consent of PCB Piezotronics Inc.

40854

	revision	S	
REV	DESCRIPTION	ECN	APP'D
NR	RELEASED TO DRAFTING		
Α	UPDATE BILL OF MATERIALS	29967	



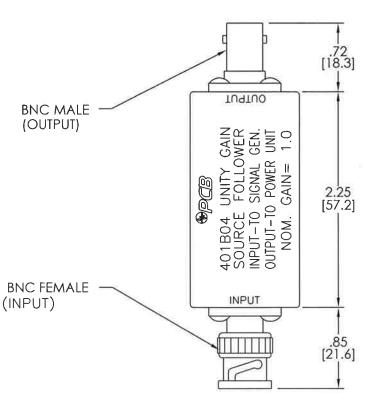



I	UNLESS SPECIF	DRAWN	
I	DIMENSIONS IN INCHES	DIMENSIONS IN MILLIMETERS [IN BRACKETS]	CHK'D
I	DECIMALS XX ±.03 XXX ±.010 ANGLES ±2 DEGREES	DECIMALS X ±0.8 XX ±0.25 ANGLES ±2 DEGREES	APP'D
İ	FILLETS AND RADII .003005	FILLETS AND RADII [0,07 - 0,13]	TITLE
I	DD011 REV D 01/17/08		I 11N

DRAWN	MCG	01/28/09	MFG	CPH	01/28/09
CHK'D	ECB	12800	ENGR	PH	01/28/09
APP'D	EB	01/28/09	SALES	MLL	01/28/09
TITLE OLITLINIE DRAWING					

OUTLINE DRAWING MODEL 401B04 UNITY GAIN SOURCE FOLLOWER

	3425 WA (716) 684	LDEN AVE.	DEPEW, I	TRONCS NY 14043 SALES@PCB.COM
1	(710) 004	0001	LIVIAIL.	SACES & L. CO.COM
4	CODE	DWG. NO.	40	0.5.4

CODE JENT. NO. 52681 40854	
----------------------------------	--


SHEET 1 OF 1


SCALE: FULL


PCB Piezotronics Inc. claims proprietary rights in the information disclosed hereon. Neither it nor any reproduction thereof will be disclosed to others without written consent of PCB Piezotronics Inc.

40854

	revision	S	
REV	DESCRIPTION	ECN	APP'D
NR	RELEASED TO DRAFTING		
Α	UPDATE BILL OF MATERIALS	29967	



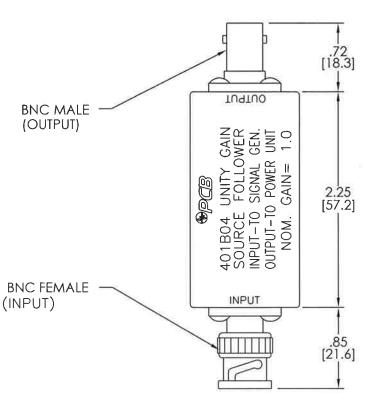



I	UNLESS SPECIF	DRAWN	
I	DIMENSIONS IN INCHES	DIMENSIONS IN MILLIMETERS [IN BRACKETS]	CHK'D
I	DECIMALS XX ±.03 XXX ±.010 ANGLES ±2 DEGREES	DECIMALS X ±0.8 XX ±0.25 ANGLES ±2 DEGREES	APP'D
İ	FILLETS AND RADII .003005	FILLETS AND RADII [0,07 - 0,13]	TITLE
I	DD011 REV D 01/17/08		I 11N

DRAWN	MCG	01/28/09	MFG	CPH	01/28/09
CHK'D	ECB	12800	ENGR	PH	01/28/09
APP'D	EB	01/28/09	SALES	MLL	01/28/09
TITLE OLITLINIE DRAWING					

OUTLINE DRAWING MODEL 401B04 UNITY GAIN SOURCE FOLLOWER

	3425 WA (716) 684	LDEN AVE.	DEPEW, I	TRONCS NY 14043 SALES@PCB.COM
1	(710) 004	0001	LIVIAIL.	SACES & L. CO.COM
4	CODE	DWG. NO.	40	0.5.4

CODE JENT. NO. 52681 40854	
----------------------------------	--

SHEET 1 OF 1

SCALE: FULL